

RH250W Hygro-Thermometer

Bluetooth® Connectivity with the ExView® Mobile App



Table of contents

1	Introduction.....	1
2	Safety	2
3	FCC Compliance	3
4	Product Description	4
	4.1 Meter Description	4
	4.2 Function Buttons	4
	4.3 Display Symbols.....	5
5	Operation	6
	5.1 Powering the Meter	6
	5.2 Auto Power Off (APO).....	6
	5.3 Taking Measurements	6
	5.4 Changing Measurement Units	7
	5.5 Data Hold Function	7
	5.6 LCD Backlight.....	7
	5.7 MAX/MIN Readings	7
	5.8 Bluetooth Operation	7
6	Maintenance.....	9
	6.1 General Cleaning	9
	6.2 Battery Replacement.....	9
7	Specifications.....	10
	7.1 General Specifications.....	10
	7.2 Measurement Specifications	10
	7.3 Environmental Specifications	10
	7.4 Connectivity Specifications	11
8	Two-year Warranty.....	12
	8.1 Calibration and Repair Services	12
	8.2 Contact Customer Support	12

1 Introduction

Thank you for selecting the Extech RH250W Hygro-Thermometer. This meter measures air temperature and relative humidity (RH) with its built-in sensor. The RH and temperature readings are shown on the top and bottom rows of the LCD, respectively.

The meter includes Bluetooth, MAX/MIN memory, selectable units of measure, auto power off, data hold, backlit LCD, and tripod mount.

Using the Extech ExView mobile app, you can pair your smart devices with the meter using Bluetooth. The app and the W Series meters were developed together for seamless integration. Download the free app from the App Store (iOS®) or from Google Play (Android™).

This quality instrument is designed to provide years of reliable service, high accuracy and simple operation. Please visit the Extech website for additional information and world-class support.

2 Safety

Please read all safety information before using this device



CAUTION

- Check for damage to the device's housing, sensor, display, and battery compartment before use. If obvious damage or abnormalities are noticed, please discontinue use and return the device for service.
- Do not attempt to open the meter or sensor. There are no user-serviceable components in this device.
- Replace the batteries immediately after the low battery symbol appears. If the device is to be stored for a period of months, please remove the batteries and store separately.
- Do not store the device in high temperature or humidity environments, in flammable or combustible areas, or where a strong electromagnetic field is present.
- This device is CE certified.

3 FCC Compliance

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

1. Reorient or relocate the receiving antenna.
2. Increase the separation between the equipment and receiver.
3. Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
4. Consult the dealer or an experienced radio/TV technician for help.




WARNING

Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

4 Product Description

4.1 Meter Description

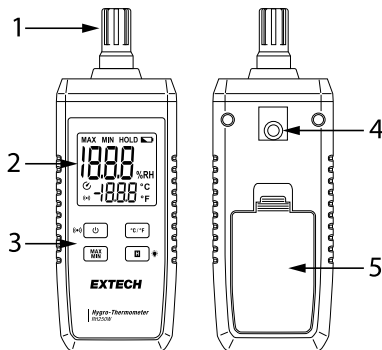


- 1. Temperature & Relative Humidity Sensor
- 2. Backlit LCD (detailed below)
- 3. Function buttons (detailed below)
- 4. Tripod mount
- 5. Battery compartment

4.2 Function Buttons

	Power / Bluetooth button Long press to switch the device on. Short press to switch off. With the meter powered, long press to switch Bluetooth on/off. Short press to switch the meter off directly from the Bluetooth mode.
	MAX/MIN button Short press to cycle through MAX/MIN readings. MAX/MIN memories are cleared each time meter power is cycled.
	Data Hold / Backlight button Short press to freeze/unfreeze the displayed reading. <i>HOLD</i> will display when data hold is active. Long press to switch the LCD backlight on/off.

°C / °F	Unit of Measure button Short press to toggle the displayed temperature units (°C / °F).
APO ON/OFF	With the meter on, long press the power and <i>H</i> buttons to switch APO on/off. The APO symbol  is displayed when APO is enabled. APO is reset each time the meter power is cycled.

4.3 Display Symbols

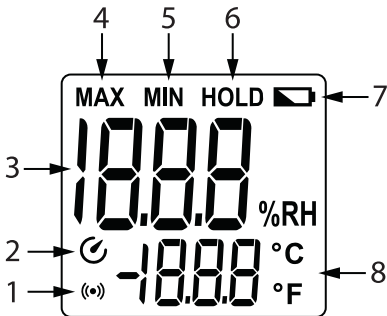

- 1. Bluetooth active
- 2. Auto Power OFF (APO) symbol
- 3. Relative Humidity reading (%RH)
- 4. Maximum reading
- 5. Minimum reading
- 6. Data Hold mode
- 7. Low battery symbol
- 8. Temperature reading with unit of measure (°C / °F)

5 Operation

5.1 Powering the Meter

The meter operates on three (3) 1.5 V (AAA) batteries, installed in the rear compartment.

Long press the power button  to switch the meter on. Short press the power button to switch the meter off. If the meter does not switch on, check the batteries for proper orientation.

When the low battery symbol  appears on the display, replace the batteries immediately to ensure accurate readings.

5.2 Auto Power Off (APO)

The meter switches off automatically five (5) minutes after the last button press.

The default mode for APO is ON (the APO symbol  on the display indicates that APO is enabled).

To switch the APO function off, with the meter switched on, long press the power  and *H* buttons. The APO symbol will switch off, indicating that the function is disabled. APO is reset each time the meter's power is cycled.

Repeat this process to switch APO back on manually.

5.3 Taking Measurements

1. Long press the power button  to switch the meter on.
2. Hold the meter in hand, set it on a table or desk, or mount it on a tripod in the area under test.
3. Read the temperature and relative humidity readings on the LCD. The RH reading is shown on the top row of the LCD in large digits. The temperature measurement is shown on the bottom row, in smaller digits.
4. If the temperature measurement is out of range, *OL* will appear on the display in place of a temperature reading. In this case, move the meter to an area congruent with the meter's measurement and operating specifications.

**CAUTION**

Do not touch or otherwise obstruct the sensor module.
Do not allow liquids to come in contact with the sensor.
Do not allow dust or other particles to enter the sensor module.

5.4 Changing Measurement Units

Short press the °C / °F button to toggle the displayed temperature units of measure.

5.5 Data Hold Function

Short press the Data Hold (*H*) button to freeze/unfreeze the displayed readings. While Data Hold is active, *HOLD* will appear on the LCD.

5.6 LCD Backlight

Long press the backlight button  to switch the display backlight on or off. Excessive use of the backlight will shorten battery life.

5.7 MAX/MIN Readings

When the device is switched on, it begins tracking the highest (MAX) and lowest (MIN) readings.

Short press the *MAX/MIN* button to step through the MAX/MIN memories. *MAX* is shown when the Maximum reading is displayed and *MIN* is shown when the Minimum reading is displayed. The memories are cleared each time the meter power is cycled.

Press the *MAX/MIN* button again to exit this mode (*MAX* and *MIN* symbols are both off when you exit).

5.8 Bluetooth Operation

Long press the Bluetooth button () with the meter on, to switch Bluetooth on or off. This communication symbol () is shown when Bluetooth is on.

The Bluetooth utility allows you to remotely monitor readings on an iOS or Android smart device using the Extech ExView mobile app designed for use with this meter.

Download the ExView mobile app from the App Store for iOS devices or from Google Play for Android devices. Instructions for mobile app use are available from the ExView product page on the Extech website (link below).

<http://www.extech.com>

Switch APO off when using Bluetooth by pressing and holding the power  and *H* buttons for 2 seconds (the APO symbol  will switch off). This will prevent the meter from automatically switching off while you are logging data or monitoring readings in real time on your smart device.

6 Maintenance



CAUTION


Warning: Do not open the housing or sensor module. Service should only be performed by factory personnel, there are no user-serviceable components in this device.

6.1 General Cleaning

Wipe the housing with a damp cloth as necessary to clean. Do not use abrasives or solvents to clean this device.

6.2 Battery Replacement

This device is powered by three (3) 1.5 V (AAA) batteries. When the low battery symbol  appears, replace the batteries immediately, as explained below.



1. Switch the meter off and remove the rear battery compartment cover.
2. Replace the batteries, observing correct polarity. Always use batteries of the same type.
3. Secure the battery compartment before use.



 Never dispose of used batteries or rechargeable batteries in household waste. As consumers, users are legally required to take used batteries to appropriate collection sites, the retail store where the batteries were purchased, or wherever batteries are sold. **Disposal:** Do not dispose of this instrument in household waste. The user is obligated to take end-of-life devices to a designated collection point for the disposal of electrical and electronic equipment.

7 Specifications

7.1 General Specifications

Display	4 digit (9999) backlit multifunction LCD
Over range indication	OL is displayed when temperature measurements are out of range
Low battery indication	Battery symbol  appears when batteries are low
Reading update rate	One reading per second
Meter power	Three (3) 1.5 V (AAA) batteries
Dimensions	137 x 55 x 28 mm (5.4 x 2.2 x 1.1 in.)
Weight	102 g (3.6 oz.)

7.2 Measurement Specifications

Accuracy specifications apply for the following conditions:

Temperature: 23°C ± 5°C (73.4°F ± 9°F); Relative Humidity: < 90 %

Temperature range	-10 to 60°C (14 to 140°F)
Temperature resolution	0.1°C (0.2°F)
Temperature accuracy	± 1.0°C (2°F)
Relative humidity range	0 to 100% RH
Relative humidity accuracy	± 5% RH

7.3 Environmental Specifications

For indoor use only

Altitude	2000 m (6562 ft.) maximum
Pollution degree	2
Operating conditions	0 to 40°C (32 to 104°F); < 90% RH
Storage conditions	-20 to 60°C (-4 to 140°F); < 75% RH
Drop-proof rating	1 m (3.3 ft.)

7.4 Connectivity Specifications

Connectivity	Bluetooth (with ExView app)
ExView app compatibility	iOS 13.0 and Android 9.0 or higher
Transmission distance	Up to 90 m (295.3 ft.) with no line-of-sight obstruction

8 Two-year Warranty

FLIR Systems, Inc. warrants this Extech brand instrument to be free of defects in parts and workmanship for **two years from date of shipment (a six-month limited warranty applies to sensors and cables). To view the full warranty text please visit: <http://www.extech.com/support/warranties>.**

8.1 Calibration and Repair Services

FLIR Systems, Inc. offers calibration and repair services for the Extech brand products we sell. We offer NIST traceable calibration for most of our products. Contact us for information on calibration and repair availability, refer to the contact information below. Annual calibrations should be performed to verify meter performance and accuracy. Product specifications are subject to change without notice. Please visit our website for the most up-to-date product information: www.extech.com.

8.2 Contact Customer Support

Customer Support Telephone List: <https://support.flir.com/contact>

Calibration, Repair, and Returns e-mail: repair@extech.com

Technical Support: <https://support.flir.com>

Website

<http://www.flir.com>

Customer support

<http://support.flir.com>

Copyright

© 2021, FLIR Systems, Inc. All rights reserved worldwide.

Disclaimer

Specifications subject to change without further notice. Models and accessories subject to regional market considerations. License procedures may apply. Products described herein may be subject to US Export Regulations. Please refer to exportquestions@flir.com with any questions.

Publ. No.: NAS100074
Release: AA
Commit: 78861
Head: 78939
Language: en-GB
Modified: 2021-08-23
Formatted: 2021-08-26